



Calibration runs, july 19


Photometer A

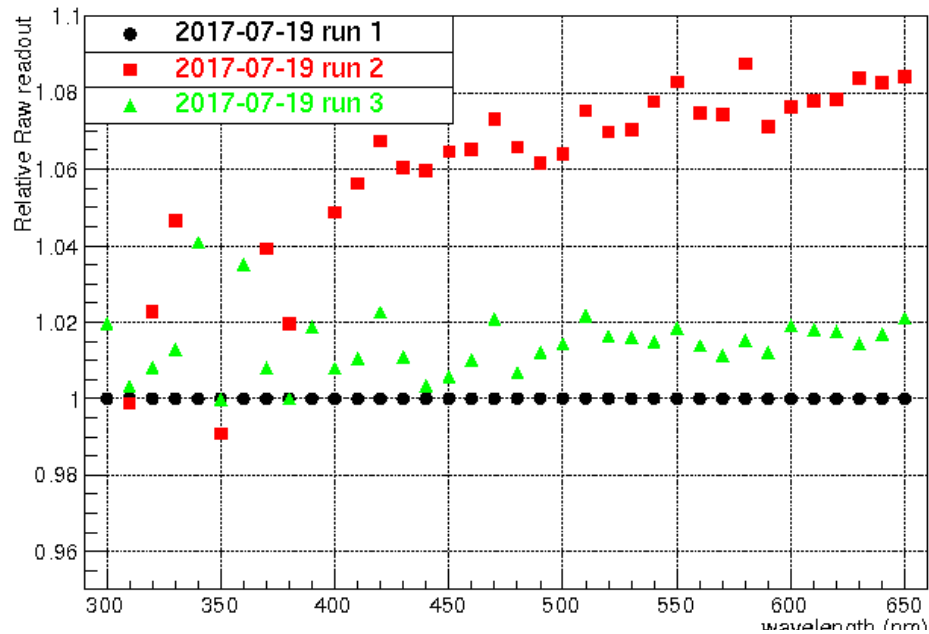

Photometer B

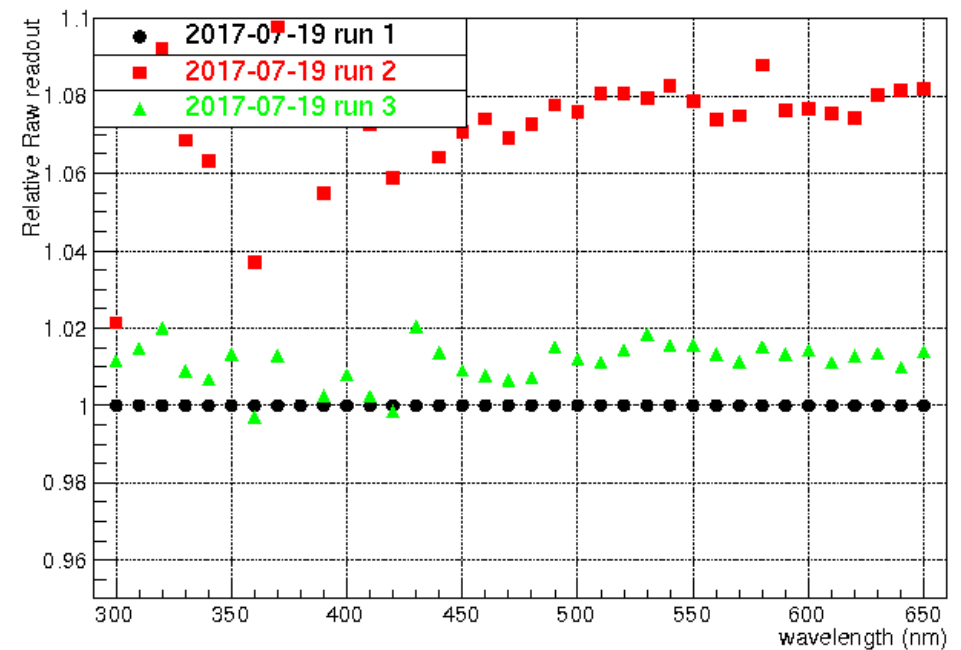


Photometer Ratio B/A

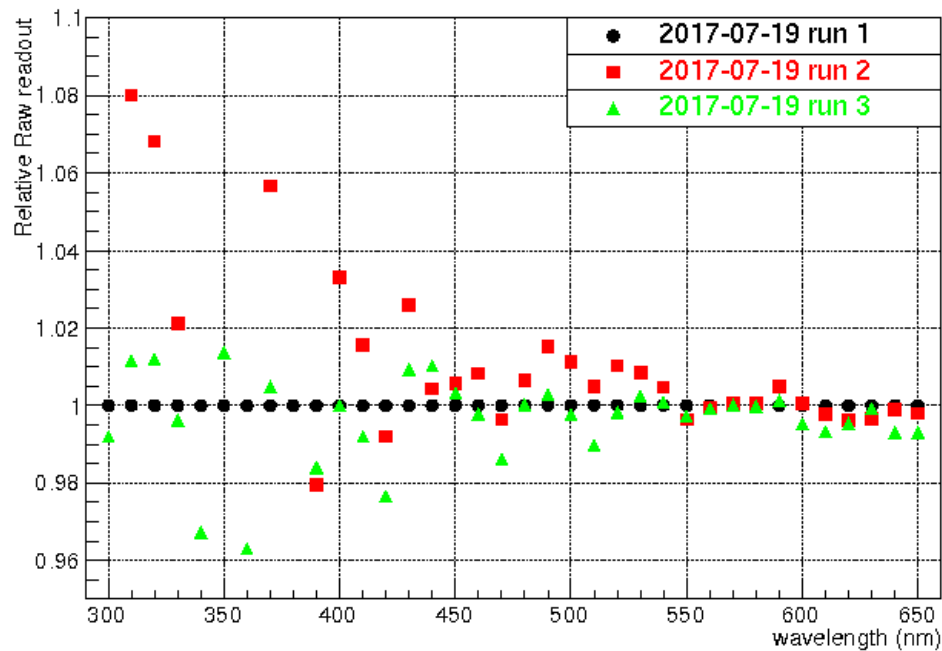


Large variations in the photodiode readout, but the ratio is stable within $\pm 2\%$ above 400 nm

Newport control mirror


Photometer A

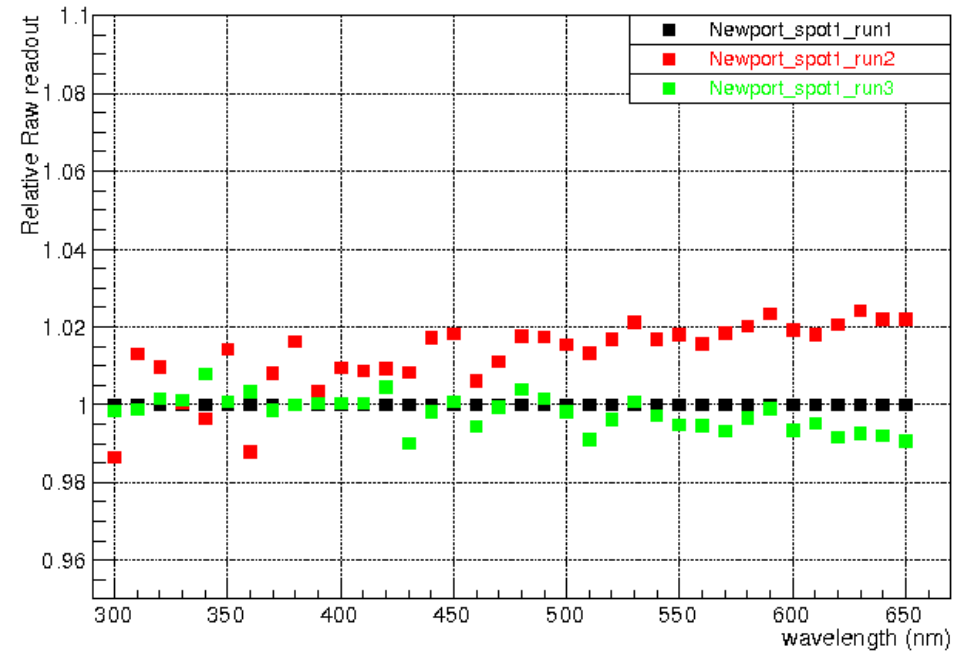

Photometer B

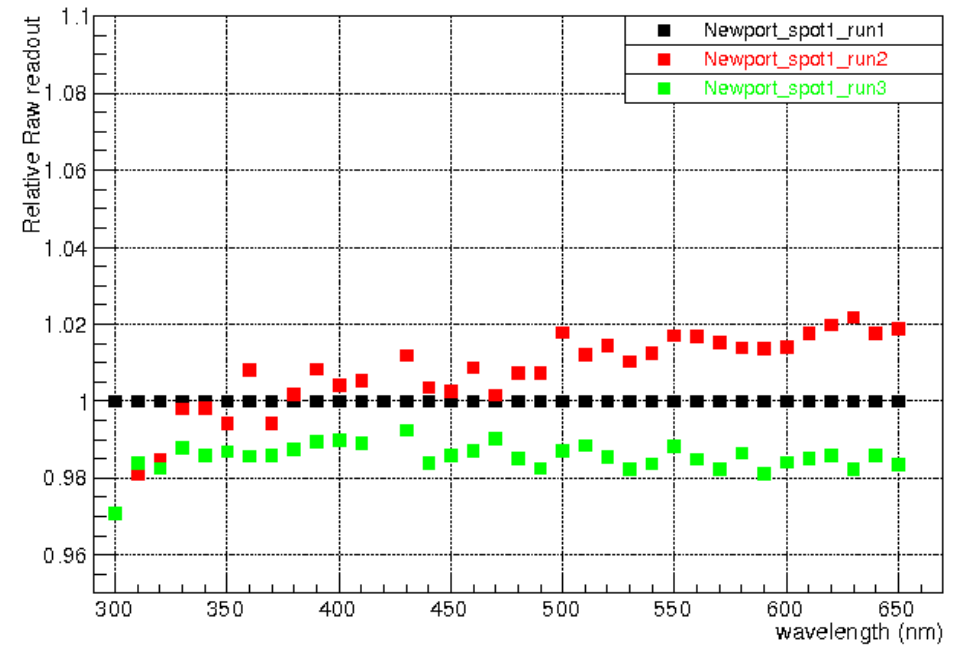

Photometer Ratio B/A

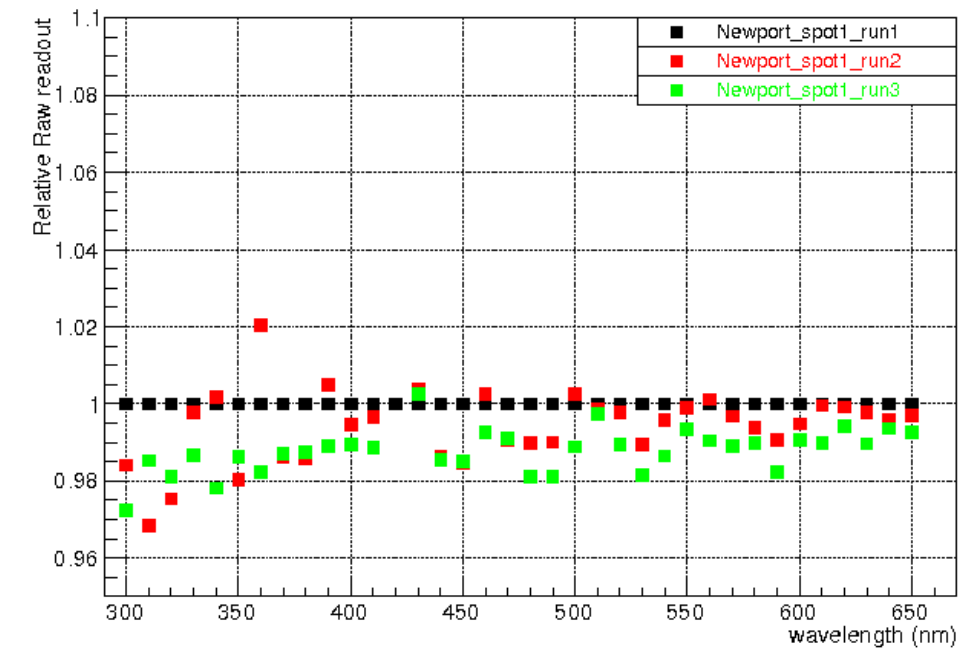


Variations in the photodiode readout smaller than in the calibration runs

The ratio is stable within $\pm 1\%$ above 400 nm

Reflectivity

Reflectivity

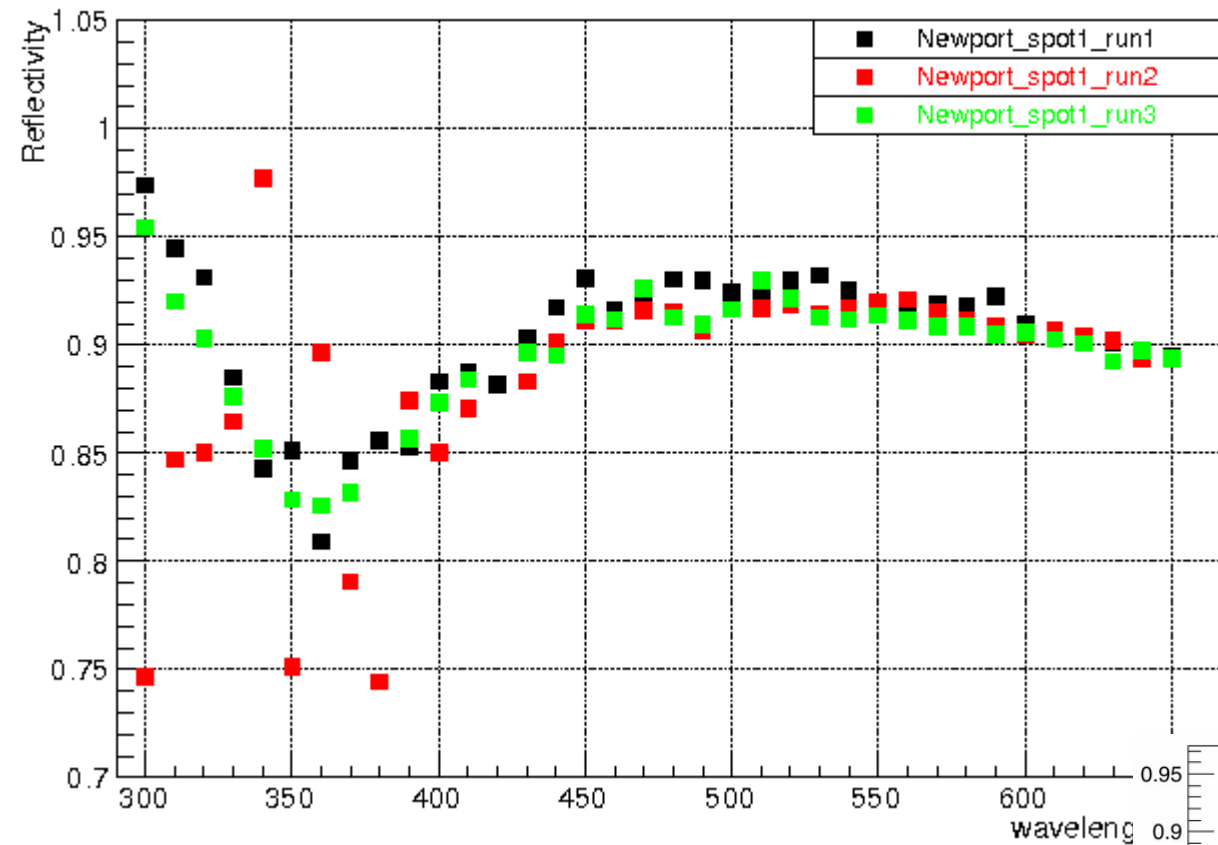

Agreement with know results

Overall, a systematic uncertainty of about $\pm 2\%$

